


Technical Specification of Bed, Hospital

S.N.	Purchaser's Specifications	Bidder's Compliance Sheet		
		Yes/ No	Ref Docs Page No.	Remarks
	Bed, Hospital			
	Manufacturer			
	Brand			
	Type/Model			
	Country of origin			
1	Description of Function			
1.1	A hospital bed is a bed specially designed for hospitalized patients in need of patient ease. These beds have special features both for the comfort and well-being of the patient .			
2	Operational Requirements			
2.1	The patient bed shall be made of solid steel construction with anti-corrosive and antirust treated baked hard epoxy powder coating.			
3	System Configuration			
3.1	Hospital Bed epoxy powder coated.			
4	Technical Specifications			
4.1	Bed base shall be anti-corrosive and antirust treated epoxy powder coated welded steel bar or epoxy powder coated 16gauge perforated sheet top to improve ventilation.			
4.2	The patient bed shall be fixed height with 2 sections where the backrest section could be elevated by mechanical hand crank located at the foot-end of the bed.			
4.3	Shall have 4 IV rod receptacles and mosquito net pole receptacles at the 4 corners.			
4.4	It shall come with one dual hook anti-corrosive and antirust treated epoxy powder coated or 304 grade stainless steel IV rod.			
4.5	Shall have bottom support of size 40x40x2.5mm square MS minimum 3 numbers per bed.			
4.6	Shall have provisions to fix urinary bag on both sides.			
4.7	All 4 legs of the hospital bed shall be capped with heavy duty rubber footings.			
4.8	Bedhead and foot-end panel (head and foot bows) shall be made of either between 4-6 anti-corrosive and antirust treated epoxy powder coated vertical tubular tube of not less than 30mm in diameter.			
4.9	Both bedhead and foot-end panel shall be detachable.			
4.10	The height of the bedhead panel: not less than 1060mm from floor.			
4.11	The height of the foot-end panel: not less than 820mm from floor.			
4.12	Overall approximate dimension: not less than 1980mm length, 910mm width, 600mm height			
4.13	The colour of the paint or coating shall be finalised during contract negotiation.			
5	System Configuration Accessories, spares and consumables			
5.1	All standard accessories/consumables/parts required for the proper operation of the above item shall be included in the offer. Bidders shall specify, in a separate Excel worksheet, the quantity and details of any items included in this offer which have not been specified in this Technical Specifications Form.			
6	Operating Environment			
6.1	The system offered shall be designed to store and to operate normally under the conditions of the purchaser's country. The conditions include Climate, Temperature, Humidity, etc.			

Umesh

Er. Umesh Kumar Chaudhary




Medical Superintendence

S.N.	Purchaser's Specifications	Bidder's Compliance Sheet		
7	Standards and Safety Requirements			
7.1	Must submit ISO13485 or better or CE certified for medical devices.			
8	Warranty			
8.1	Warranty for 2 year.			
9	Maintenance Service During Warranty Period			
9.1	Standard warranty conditions are applicable. Breakdown maintenance shall be done by supplier during warranty period.			
10	Installation and Commissioning			
10.1	Must supply preassembled unit, ready to use.			
11	Documentation			
11.1	Users/Instructions manual shall be provided in English.			

Bidder must completely fill the Technical Specification Form (TSF). Only Yes/no/all complies should not be written. Page number in the catalogue of all the required parameters must be clearly mentioned and highlighted. Failure in doing so may lead to rejection of bid from technical committee

[Signature]
K. P. Kumar Choudhary
 NEC No.: 162-Biomedical A

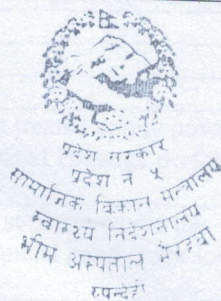

[Signature]
मेडिकल सुपरिटेन्डेंट